


Quick Guide for CO₂ Waveforms

PROPAQ[®] Vital Signs Monitors


This Guide is intended for quick reference only. It is strongly recommended that clinicians new to capnography also refer to published educational literature on this subject.

All waveform illustrations in this guide apply to both **Mainstream CO₂** and **Sidestream CO₂** with intubated patients. Mainstream CO₂ waveforms tend to be slightly more defined, especially on the upstroke, plateau, downstroke; Sidestream CO₂ waveforms are more rounded.

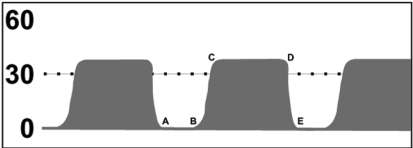

WelchAllyn[®]


The Normal CO₂ Waveform

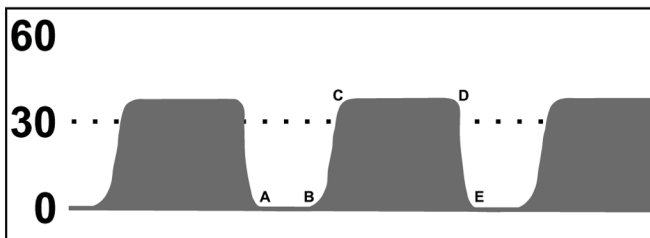

The “normal” capnogram shape consists of the following:

- A-B** **Zero baseline** – the beginning of exhalation
- B-C** **Rapid, sharp rise** – anatomical dead space gas replaced by more distal airway gases that contain more CO₂
- C-D** **Alveolar “plateau”** – contains mixed alveolar gases
- D** **End-Tidal CO₂** – highest concentration of exhaled CO₂
- D-E** **Rapid, sharp downstroke** – inhalation phase; fresh gas rapidly replaces CO₂


Endotracheal Tube In Esophagus

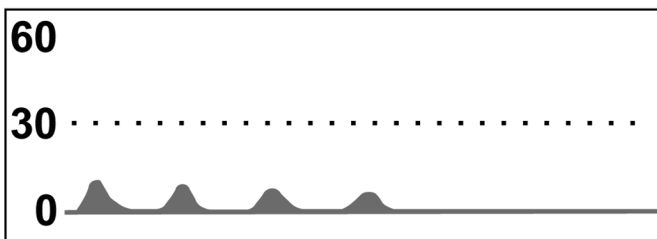

If inadvertent esophageal intubation occurs, the capnogram indicates the endotracheal tube is incorrectly positioned and ventilation is not taking place. Look for:

- No CO₂ measured
- Only small, short-lived capnograms displayed


Endotracheal Tube “Leaks”

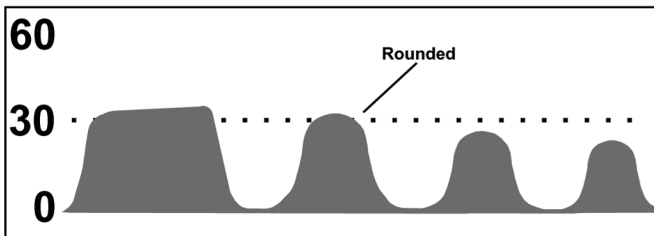

If air leaks around the endotracheal tube cuff, the alveolar (end-tidal) CO_2 gas is diluted. The alveolar plateau is blunted, and it blends with the downstroke of the capnogram. Look for:

- A deflated or leaky endotracheal or tracheal tube cuff
- An artificial airway that is too small for the patient


Decreased Muscle Relaxant Effect Or Breathing Against Ventilator

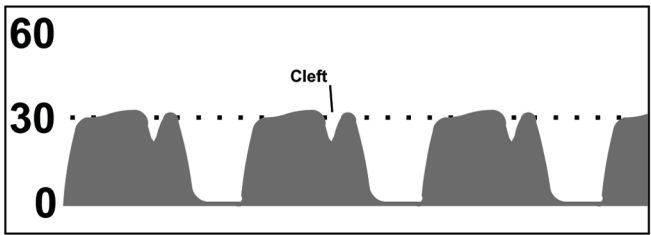

The “cleft” in the far right portion of the alveolar plateau indicates that the diaphragm is moving and causing entrainment of fresh air. A cleft can occur in any part of the alveolar plateau when the patient attempts to breath against the ventilator. Look for:

- Clefts in the capnogram (may not be on every waveform)
- “Humped” waveforms (indicating attempts at spontaneous breathing)


Endotracheal Tube Kinked Or Airway Obstructed

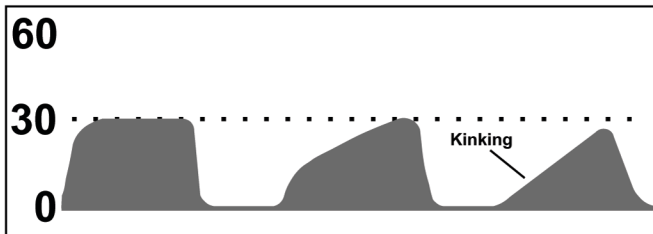

If exhaled CO₂ gas is completely or partially obstructed, the slope of the ascending limb of the capnogram has little or no alveolar plateau. Look for:

- Partially kinked or occluded artificial airway
- Herniated endotracheal or tracheal tube cuff
- Bronchospasm, chronic obstructive pulmonary disease
- Foreign body in the upper airway

Rebreathing CO₂

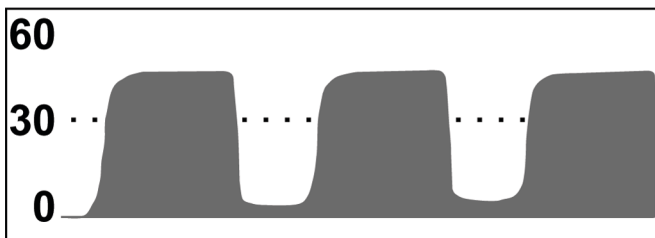

If the patient is rebreathing previously exhaled CO₂, ETCO₂ values increase and the baseline elevates. The waveform does not return to zero at the end of inspiration. Look for:

- Inadequate expiratory time
- Malfunctioning inspiratory valve
- Other errors/malfunctions in breathing circuit
- Insufficient inspiratory flow rate

WelchAllyn®

Beaverton, Oregon USA

Within USA, toll free:

Phone: (800) 289-2500

Phone Technical Services: (800) 289-2501

WorldWide: Phone: (1) 503 526-8500

Fax: (1) 503 526-4200

Fax Technical Services: (1) 503 526-4910

©2001 Printed in USA
P/N: 810-0466-02 Rev A 11/01